

J-KEM Scientific, Inc.
Instruments for Science from Scientists

J-KEM® Scientific, Inc.
6970 Olive Blvd.
St. Louis, MO 63130
(314) 863-5536
Fax (314) 863-6070
E-Mail: jkem911@jkem.com

Nitrogen Gas Heater

Warranty

J-KEM Scientific, Inc. warrants this unit to be free of defects in materials and workmanship and to give satisfactory service for a period of 12 months from date of purchase. If the unit should malfunction, it must be returned to the factory for evaluation. If the unit is found to be defective upon examination by J-KEM, it will be repaired or replaced at no charge. However, this WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of being damaged as a result of excessive current, heat, moisture, vibration, corrosive materials, or misuse. This WARRANTY is VOID if devices other than the reaction block supplied with this unit are powered by the controller. Components which wear or are damaged by misuse are not warranted. This includes contact points, fuses and solid state relays.

THERE ARE NO WARRANTIES EXCEPT AS STATED HEREIN. THERE ARE NO OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND OF FITNESS FOR A PARTICULAR PURPOSE. IN NO EVENT SHALL J-KEM SCIENTIFIC, INC. BE LIABLE FOR CONSEQUENTIAL, INCIDENTAL OR SPECIAL DAMAGES. THE BUYER'S SOLE REMEDY FOR ANY BREACH OF THIS AGREEMENT BY J-KEM SCIENTIFIC, INC. OR ANY BREACH OF ANY WARRANTY BY J-KEM SCIENTIFIC, INC. SHALL NOT EXCEED THE PURCHASE PRICE PAID BY THE PURCHASER TO J-KEM SCIENTIFIC, INC. FOR THE UNIT OR UNITS OF EQUIPMENT DIRECTLY AFFECTED BY SUCH BREACH.

J-KEM Scientific, Inc.
6970 Olive Boulevard
St. Louis, MO 63130
USA

Phone: (314) 863-5536
FAX: (314) 863-6070
Web site: <http://www.jkem.com>
E-Mail: jkem911@jkem.com

Safety Notices

Solvents and Vapors

J-KEM's Nitrogen gas heater must not be used in an environment containing flammable organic reagents or gas vapors. Any inert gas can be used with the gas heater, such as nitrogen or argon. No flammable reagents of any nature or reactive gasses, such as oxygen, can be used with this heater. CAUTION: This equipment should only be operated by qualified personnel knowledgeable in laboratory procedures.

Symbols

Power Switch: 1 - Mains power is ON.
0 - Mains power is OFF.



Caution. Risk of electric shock.



Caution. No user serviceable parts.



Protective conductor terminal. Earth Ground.

General Notice

WARNING: If equipment is not used as specified in this manual, the protection provided by this equipment may be impaired.

CAUTION: When operating this equipment insure that the heater is located away from flammable object.

Power

	120 Vac Input Version	220-240 Vac Input Version
Voltage	120 VAC @ 50-60Hz	230 VAC @ 50-60Hz
Wattage	600 watts; 5 amps.	600 watts; 2.5 amps.
Fusing	5 amp fast acting (F) 120 vac fuses	4 amp fast acting (F) 230 vac fuses

Environmental

Indoor use


Altitude up to 2000 meters

Operating temperatures of 5° C to 40° C

Maximum relative humidity of 80% for temperature up to 31° C decreasing linearly to 50% relative humidity at 40° C.

Installation category II

Controller Description

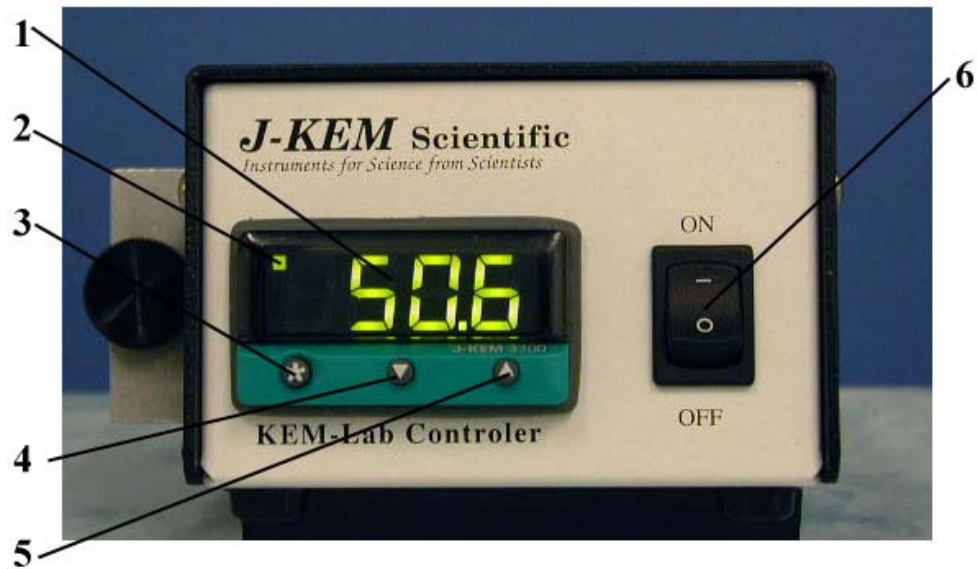

1. Temperature Display. Shows temperature of the exit gas as the default display. Shows set point temperature (i.e. desired temperature) as a blinking number when ‘*’ button is held in.
2. Indicates that heating power is being applied to the heater when lit.
3. Control Key. When held in, the display shows the set point temperature. To decrease or increase the set point, press the ‘▼’ key (4) or ‘▲’ key (5), while simultaneously holding in the control key. The set point appears as a blinking number in the display.
4. Lowers set point when ‘*’ button (3) is simultaneously pressed.
5. Raises set point when ‘*’ button (3) is simultaneously pressed.
6. Controller On/Off switch.

Connecting Gas to the Gas Heater

The gas heater has a gas inlet and outlet with no other connections. Connect inlet gas to the port labeled IN which is the port on the same side of the heater that the power cord from the temperature controller connects to. The heated gas outlet is on the side of the controller labeled OUT.



Before turning the temperature controller on, the gas heater MUST:


1. Have gas entering on the port labeled “IN” and exiting on the port labeled “OUT”, and
2. nitrogen gas must be flowing through the heater at a minimum flow rate of 1 liter per minute.

Failure at either of these points will burn the heater out and void the warranty..

Entering a Setpoint into the Controller

1. Turn on gas flow into the heater to a minimum flow rate of 500ml/min.

2. Turn power on to the digital temperature controller. The default display (when no buttons are being pressed) of the controller is the current oven temperature.

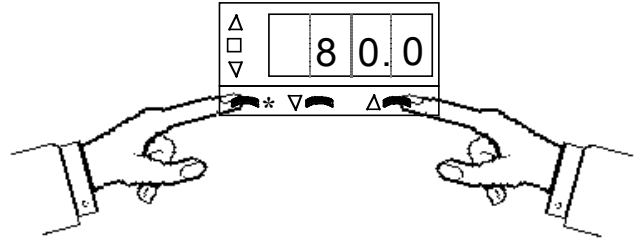

3. To see the current setpoint temperature (i.e., the desired temperature), press and hold in the ‘*’ button on the front of the digital meter. The current setpoint appears as a blinking number in the display. To enter a new setpoint, hold in the ‘*’ button on the front of the meter. While holding in the ‘*’ button press either the ▲ button to increase, or the ▼ button to decrease the setpoint. When the desired temperature is present in the display, release all the buttons.